

# Radial Profile Measurements of Electron Temperature and Density Using the Thomson Scattering System in GAMMA 10/PDX<sup>\*)</sup>

Masayuki YOSHIKAWA, Junko KOHAGURA, Masayuki CHIKATSU, Yoriko SHIMA, Mizuki SAKAMOTO, Yousuke NAKASHIMA, Ryutaro MINAMI, Ichihiko YAMADA<sup>1)</sup>, Ryo YASUHARA<sup>1)</sup>, Hisamichi FUNABA<sup>1)</sup>, Takashi MINAMI<sup>2)</sup> and Naoki KENMOCHI<sup>3)</sup>

*Plasma Research Center, University of Tsukuba, 1-1-1 Tennodai, Tsukuba, Ibaraki 305-8577, Japan*

<sup>1)</sup>*National Institute for Fusion Science, 322-6 Oroshi-cho, Toki, Gifu 509-5292, Japan*

<sup>2)</sup>*Institute of Advanced Energy, Kyoto University, Gokasho, Uji, Kyoto 611-0011, Japan*

<sup>3)</sup>*Graduate School of Frontier Sciences, University of Tokyo, Kashiwa, Chiba 277-8561, Japan*

(Received 21 December 2017 / Accepted 28 March 2018)

We developed the YAG Thomson scattering (TS) system for electron temperature and density radial profiles in a single laser shot in the tandem mirror GAMMA 10/PDX. The optical collection system for the TS light is constructed using spherical mirrors and nine bundled optical fibers. The measurable radial positions are 5-cm intervals in a region of  $\pm 20$  cm due to the fixed position of the bundled optical fibers, which are set on a fixed-height optical platform. We replaced this with a lab jack to make the bundled optical fiber positions movable. Consequently, we can measure the radial profiles of the electron temperature in more detail. Moreover, we added a third spherical light collection mirror at the bottom of the main spherical collection mirror to increase the TS light intensity in the edge plasma region. In this way, we can obtain a slightly larger TS signal intensity than in the case without a third collection mirror. The radial electron temperatures and densities at 15 radial positions in GAMMA 10/PDX are successfully obtained. For the in-situ calibration of the electron density measurements of the TS system, we compare the TS system measurements to the electron line density measured using a microwave interferometer system.

© 2018 The Japan Society of Plasma Science and Nuclear Fusion Research

Keywords: Thomson scattering, radial profile, electron temperature, electron density, tandem mirror GAMMA 10/PDX

DOI: 10.1585/pfr.13.3402051

## 1. Introduction

Thomson scattering (TS) is the most useful diagnostic available to measure the electron temperature and density in fusion devices [1–10]. To apply a TS system in lower electron density plasmas, such as GAMMA 10/PDX and the spherical region of fusion plasmas, large numerical aperture collection optics and large scattering lengths are required. In GAMMA 10/PDX, we installed an yttrium-aluminum-garnet (YAG)-TS system with large angle collection optics and a large scattering length optical system [8, 9]. The YAG-TS system can measure radial electron temperatures and densities at seven fixed positions in a single laser shot at 10 Hz. GAMMA 10/PDX is effectively an axisymmetric minimum-B anchored tandem mirror with a thermal barrier at both end-mirrors [11]. The  $x$ - and  $y$ -axes are perpendicular to the magnetic field in the vertical and horizontal directions, respectively. The  $z$ -axis is parallel to the magnetic field. The plasma is created by plasma guns and heated and sustained using ion cyclotron heating (ICH) systems. In addition to ICH, electron cy-

clotron heating (ECH) is applied to produce the electron and ion confinement potential in the plug (P) and barrier (B) cells. In the central cell, we performed direct electron heating by applying the central (C) ECH [12]. Super molecular beam injection (SMBI) experiments have been performed in the central cell to increase the plasma density and to create the higher end loss flux for divertor plasma experiments [13]. In the end region, we installed a divertor simulation experimental module to perform the divertor simulation experiments. The electron density, electron temperature, and ion temperature are measured using the YAG-TS system, microwave interferometers, a soft X-ray measurement system, and a charge exchange neutral particle analyzer system [14–17]. The typical electron density and electron and ion temperatures are approximately  $2 \times 10^{12} \text{ cm}^{-3}$ , 100 eV, and 5 keV, respectively, during the application of P/B-ECH.

The optical collection system for the TS light is constructed using spherical mirrors and nine bundled optical fibers. The measurable radial positions are 5-cm intervals in the region of  $\pm 20$  cm due to the fixed position of the bundled optical fibers, which are set on a fixed-height optical platform. The e-folding radius of the C-ECH power

author's e-mail: yosikawa@prc.tsukuba.ac.jp

<sup>\*)</sup> This article is based on the presentation at the 26th International Toki Conference (ITC26).

density of the radiation distribution on the resonance surface is approximately 3 cm, and the FWHM of the  $x$ -axis  $H\alpha$  emission radial profile on the SMBI experiment is approximately 6 cm just after the injection to the plasma. To measure the radial TS signals in more detail, less than a 5-cm interval, we replaced the fixed-height optical platform with a lab jack to make the bundled optical fiber position movable. Moreover, we added a third spherical light collection mirror at the bottom of the main spherical collection mirror to increase the TS light intensity in the upper side edge plasma region. These improvements will be useful for studying the heating mechanisms of the C-ECH and SMBI experiments. During the GAMMA 10/PDX plasma experiments, we sometimes need to change the optical components after performing the density calibration gas scattering experiments due to damage to the optical components or to reset the optical systems to improve the scattering signal intensity. For the in-situ calibration of the electron density measurements of the TS system, we compare the measurements to the electron line density measured by the 6-channel microwave interferometer (MIF) system [16, 17].

In this paper, we demonstrate the improved YAG-TS system for measuring the detailed radial profiles of electron temperatures and densities with the newly installed lab jack system and third additional collection mirror after performing in-situ calibration using the microwave interferometer system in the central cell of GAMMA 10/PDX.

## 2. Experimental Apparatus

The YAG-TS system installed at  $z = 60$  cm in the GAMMA 10/PDX central cell is shown in Fig. 1. The YAG-TS system is composed of a laser, incident optics, light collection optics, signal detection electronics, and a data recording system. A 10-Hz Nd:YAG laser (Continuum, Powerlite 9010) with an energy per pulse of 2 J and a pulse width of approximately 10 ns operating at the fundamental wavelength of 1064 nm is used. The laser goes

through a short pass half mirror, two Faraday rotators, two polarizers, two  $\lambda/2$  plates, four mirrors, and an iris on the optical bench. The laser beam is injected into the plasma from the down side port through a focusing lens of  $f = 2.25$  m. The laser beam diameter at the plasma center is approximately 1 mm. The polarization of the laser in the plasma is in the  $z$ -direction. The light collection optics were optimized with the help of optical system design software (ZEMAX). For the light collection optics, we used a spherical mirror with an Al:SiO<sub>2</sub> coating, a curvature radius of 1.2 m, and a diameter of 0.6 m. For the down side edge plasma light collection, we set a second spherical mirror with a curvature radius of 1.2 m and a diameter of 0.2 m on the top of the main spherical mirror [10]. The additional mirror system is useful for increasing the TS signal from the edge plasma in the TS system. Moreover, we added a third collection mirror with a curvature radius of 1.0 m and a rectangular size of 0.12 m  $\times$  0.30 m set at the down side of the main spherical mirror to double the TS light from the upper side edge plasma region. The distance between the main mirror center and the additional mirror center is approximately 0.34 m. The mirror size is optimal for obtaining the maximum collection efficiency, considering the solid angle and the setting position. The scattered light is collected by the spherical mirrors, reflected, and reaches a bundled optical fiber with a cross section of 2 mm  $\times$  7 mm. The magnification of the collection optics is 1/2.2. The length of the scattering volume along the laser is 15.4 mm, and the scattering angle is 90°. A solid angle of 0.078 sr can be realized by the light collection optics of the main collection mirror. After passing through the plasma, the laser beam is ejected from the upper side port and absorbed by the beam dump through the mirror flipper system. The 6.67-m-long bundled optical fiber (Mitsubishi Densen, FS10-43001A) is connected to a 5-channel polychromator. The bundled optical fiber has a very large numerical aperture of approximately 0.47. The fiber aperture should be located approximately 0.873 m from the spherical mirror. The fiber positions were fixed by the fiber slot on the fixed-high optical platform. The measurable radial positions are 5-cm intervals in the region of  $\pm 20$  cm. To measure the radial TS signals in intervals of less than 5 cm, we replaced the fixed-height optical platform with a lab jack (Thorlabs, L490) to make the bundled optical fiber position movable. The polychromator is composed of five relay and collection lenses, five interference filters, and five silicon avalanche photodiodes (Si-APD, PerkinElmer, C30950E and C30659-1060-3AH). Four-channel high-speed oscilloscopes (IWATSU, DS5524, and DS5524A) were used to measure four wavelength channels simultaneously with a bandwidth of 200 MHz and a sampling rate of 1 GS/s at 10 Hz. The measured signals are recorded by a Windows PC with LabVIEW analyzing software. We conducted wavelength calibration experiments of the spectral sensitivities of the 5-channel polychromators using a standard

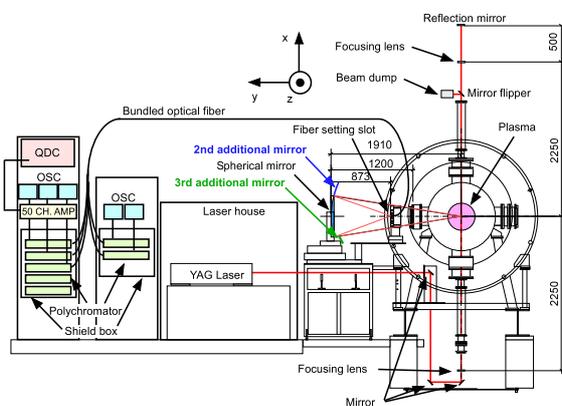


Fig. 1 Side view of the TS system in the GAMMA 10 central cell.



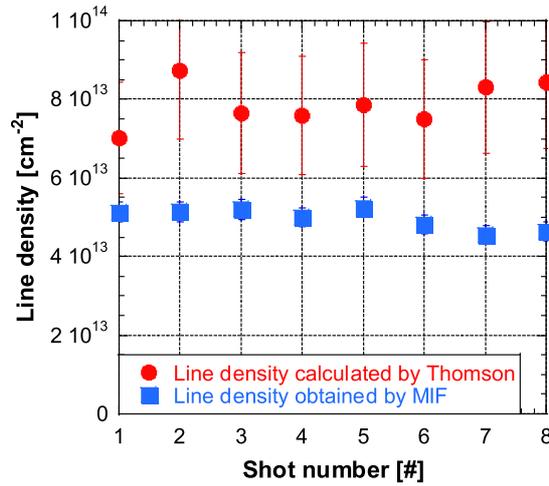


Fig. 4 Comparison of the line densities measured using the MIF and TS systems.

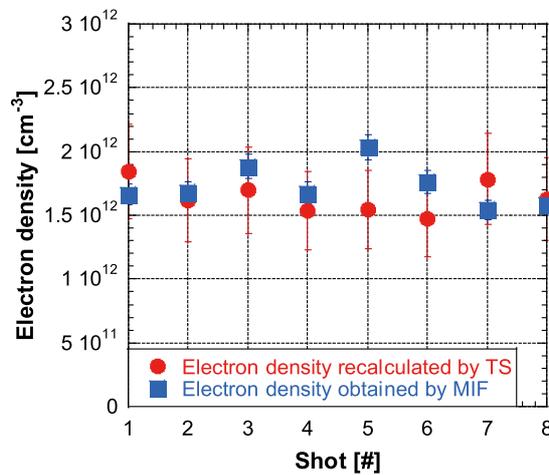


Fig. 5 Comparison of the electron densities obtained using the MIF and in-situ calibrated TS systems.

squares) in the same eight plasma shots. Every electron line density in Fig. 4 was obtained in a single plasma shot by the TS and 6-channel MIF systems. The averaged ratio of the integrated line densities obtained by the TS system and those obtained by the MIF system is approximately 1.6. In Fig. 5, we show the electron densities obtained by the 6-channel MIF system (blue closed squares) and the in-situ calibrated TS system (red closed circles) divided by the above ratio. After the calibration, the TS measured electron density is the same as that calculated by the 6-channel MIF system within an error of 20% for every shot. We can compare the measurements shot-by-shot to check the total sensitivity of the TS system. The calibration coefficients changed a little after some system adjustments of the TS system and the YAG laser intensity.

Figures 6(a) and 6(b) show the radial electron temperature and density profiles measured using the TS system at  $t = 155.1$  ms when changing the measuring positions by

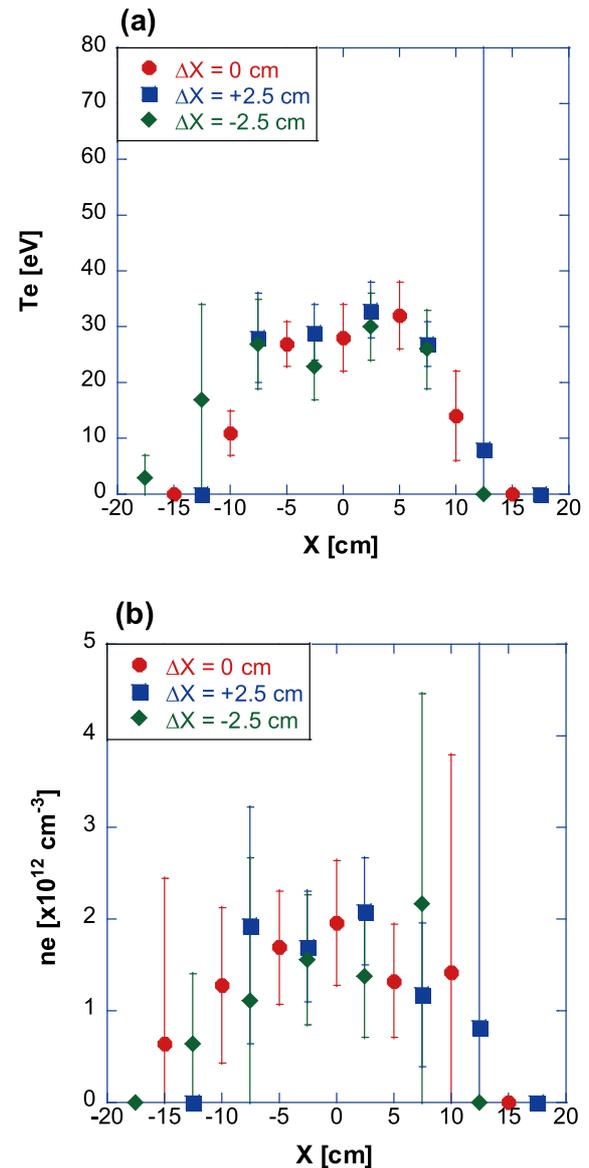


Fig. 6 Radial profiles of (a) the electron temperature and (b) the density when changing the lab jack position.

$\pm 2.5$  cm from the base position of the lab jack shot-by-shot in three plasma shots, respectively. Here, the red closed circles, blue closed squares, and green diamonds show the results at  $\Delta X = 0$  cm,  $+2.5$  cm, and  $-2.5$  cm from the base position of the lab jack, respectively. Then, we measured the radial positions of the electron temperature and density in 2.5-cm intervals.

## 5. Summary

We added a third collection mirror to improve the TS signals from the edge region plasma; this increased the TS signal intensity slightly; however, we need to further optimize the mirror setting. The detailed radial electron temperature and density profiles were successfully measured using the newly installed lab jack system. In addition, we used an in-situ calibration comparing the mea-

sured line density using the microwave interferometer system and calculated the line density using the electron densities from the YAG-TS system.

## Acknowledgments

The authors thank the members of the GAMMA 10/PDX group of the University of Tsukuba for their collaboration. This study was conducted with the support and under the auspices of the NIFS Collaborative Research Program (NIFS11KUGM056) and the Bidirectional Collaboration Research Programs (NIFS14KUGM086, NIFS14KUGM088).

- [1] K. Narihara *et al.*, *Fusion Eng. Des.* **34-35**, 67 (1997).
- [2] J.H. Foote *et al.*, *Rev. Sci. Instrum.* **61**, 2861 (1990).
- [3] J. Hatae *et al.*, *Rev. Sci. Instrum.* **70**, 772 (1999).
- [4] T. Hatae *et al.*, *Rev. Sci. Instrum.* **77**, 10E508 (2006).
- [5] J. Hiratsuka *et al.*, *Plasma Fusion Res.* **5**, 044 (2010).
- [6] H. Togashi *et al.*, *Plasma Fusion Res.* **9**, 1202005 (2014).
- [7] M. Yu Kantor *et al.*, *Plasma Phys. Control. Fusion* **51**, 055002 (2009).
- [8] M. Yoshikawa *et al.*, *Plasma Fusion Res.* **6**, 1202095 (2011).
- [9] M. Yoshikawa *et al.*, *J. Instrum.* **8**, C10016 (2013).
- [10] M. Yoshikawa *et al.*, *J. Instrum.* **10**, C11006 (2015).
- [11] Y. Nakashima *et al.*, *Nucl. Fusion* **57**, 116033 (2017).
- [12] R. Minami *et al.*, *Trans. Fusion Sci. Technol.* **59**, 244 (2011).
- [13] Md. M. Islam *et al.*, *Plasma Fusion Res.* **11**, 2402053 (2016).
- [14] M. Yoshikawa *et al.*, *Plasma Fusion Res.* **8**, 1205169 (2013).
- [15] M. Yoshikawa *et al.*, *Plasma Fusion Res.* **9**, 1202126 (2014).
- [16] M. Yoshikawa *et al.*, *Rev. Sci. Instrum.* **79**, 10E706 (2008).
- [17] Y. Hasegawa *et al.*, *Trans. Fusion Sci. Technol.* **63**, 337 (2013).